

HETEK FLOW SAMPLER

Quick Operation Guide/ Prise en main rapide



Switch On / Mise en marche



HETEK FLOW SAMPLER
FIRMWARE VERSION : 1.00

08/05/2022 9:37:41 100%
CALIBRATION DUE IN : 30 DAYS


08/05/2022 9:37:41 100%
PURGING SENSORS
PLEASE WAIT...



Bump Test / Test de vérification

08/05/2022 9:37:41 100%
1. VERIFY
2. CALIBRATE SENSOR
3. ERASE PREVIOUS CAL. LOG
4. ERASE ENTIRE CAL. LOG
1. VERIFY


08/05/2022 9:37:41 100%
VERIFY
LEAK (%) 100.00
BACK (%) 100.00
ENTER = VERIFY ESC. = EXIT

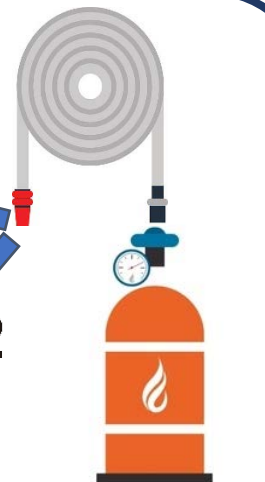

Methane



User Manual / Manuel d'utilisation



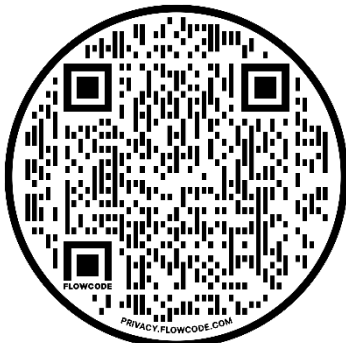


www.hetek.com

Settings / Paramètres

08/05/2022 9:37:41 100%
1. FLOW UNITS 5. PURGE
2. TEMP. UNITS 6. ERASE DATA LOG
3. CALIBRATION 7. SET TIME/DATE
4. DATA UPLOAD 8. ACCESS RECORDS
1. FLOW UNITS

Start Test / Opération

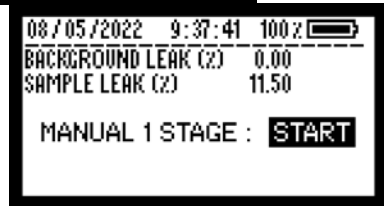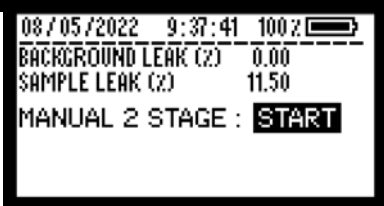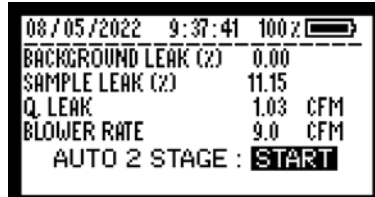

Charging / Mise en charge



12h



Data Download / Téléchargement de données



Switch Off / Mise à l'arrêt



Manufactured in Canada / Fabriqué au Canada